

FIG. 1

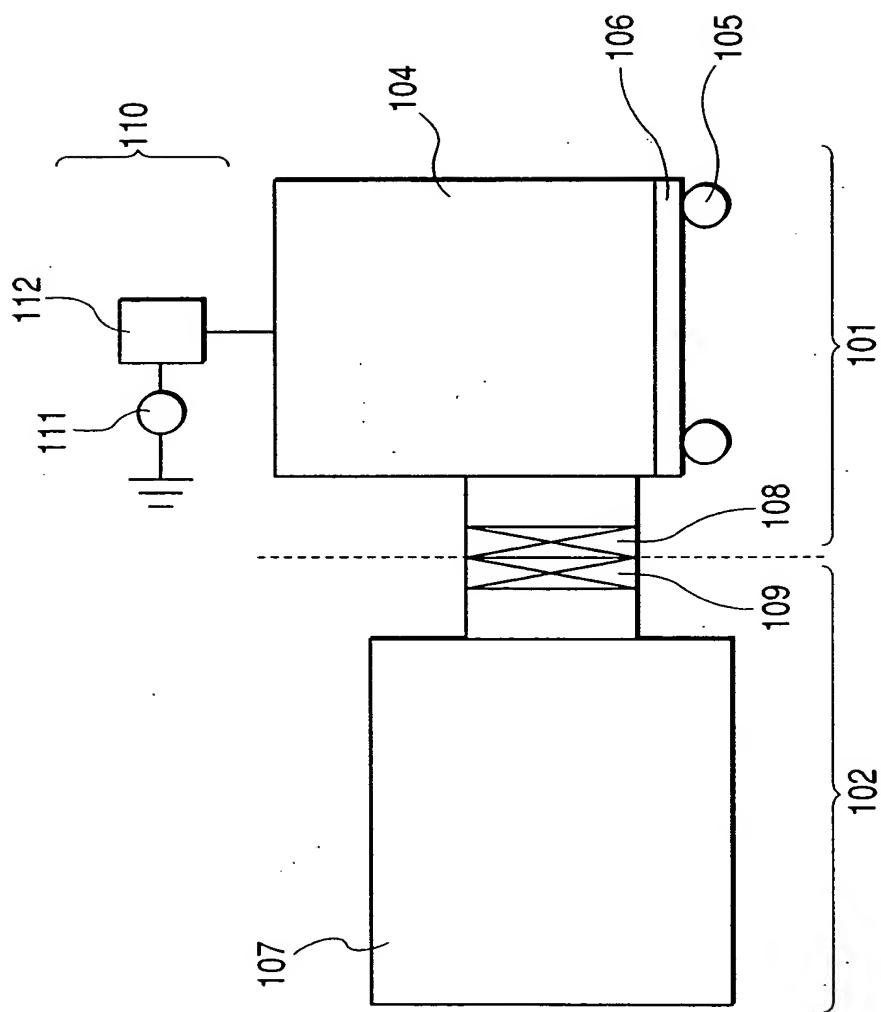


FIG. 2

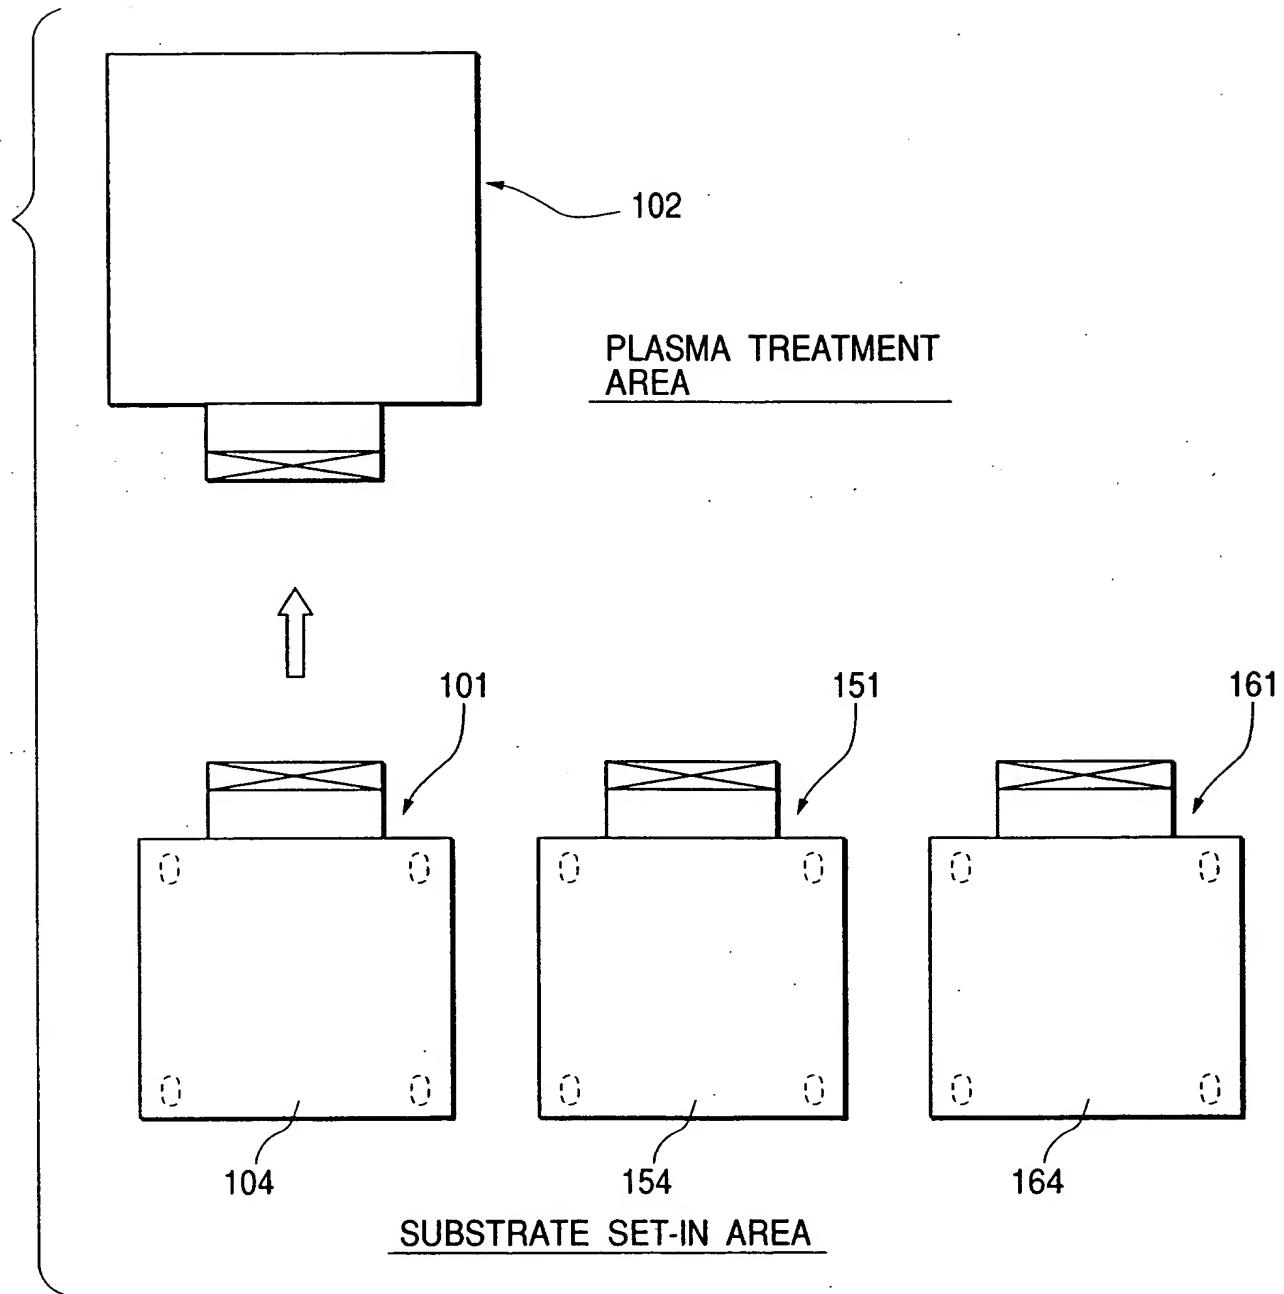


FIG. 3

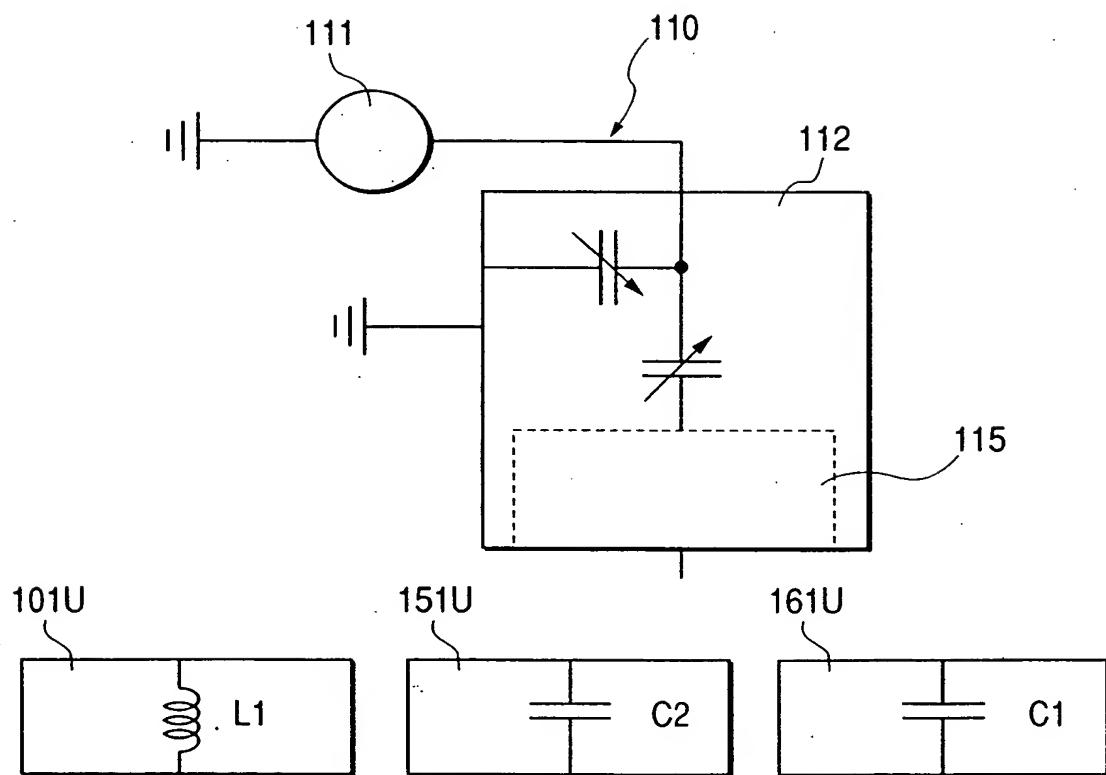


FIG. 4

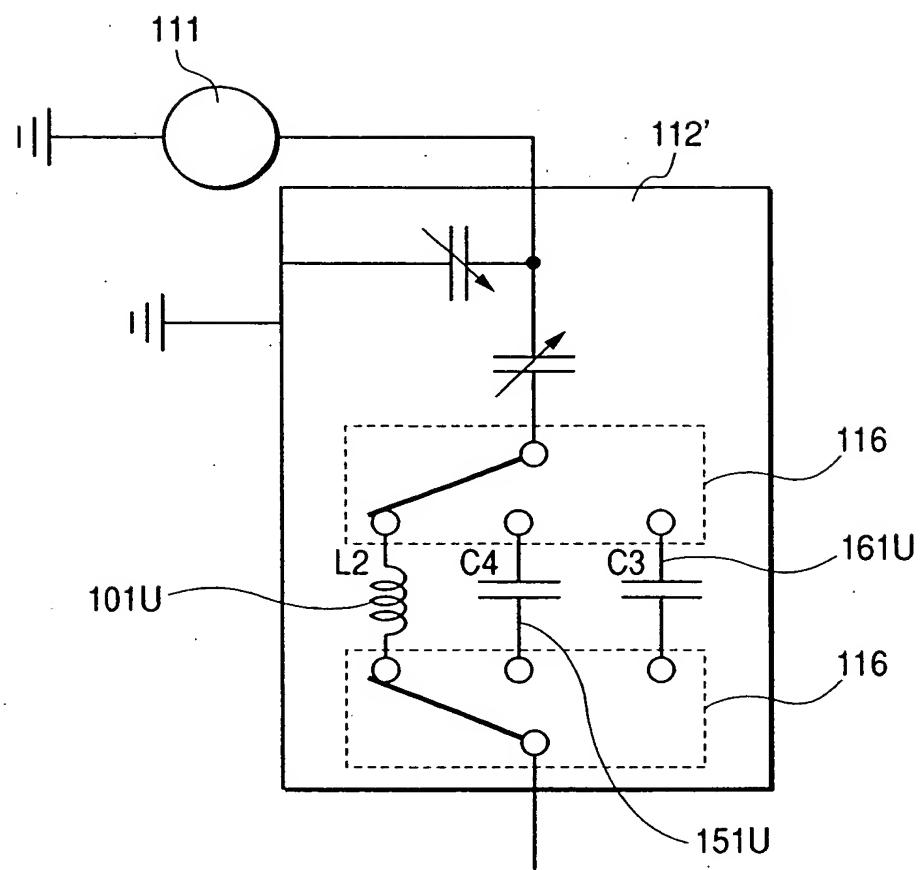


FIG. 5

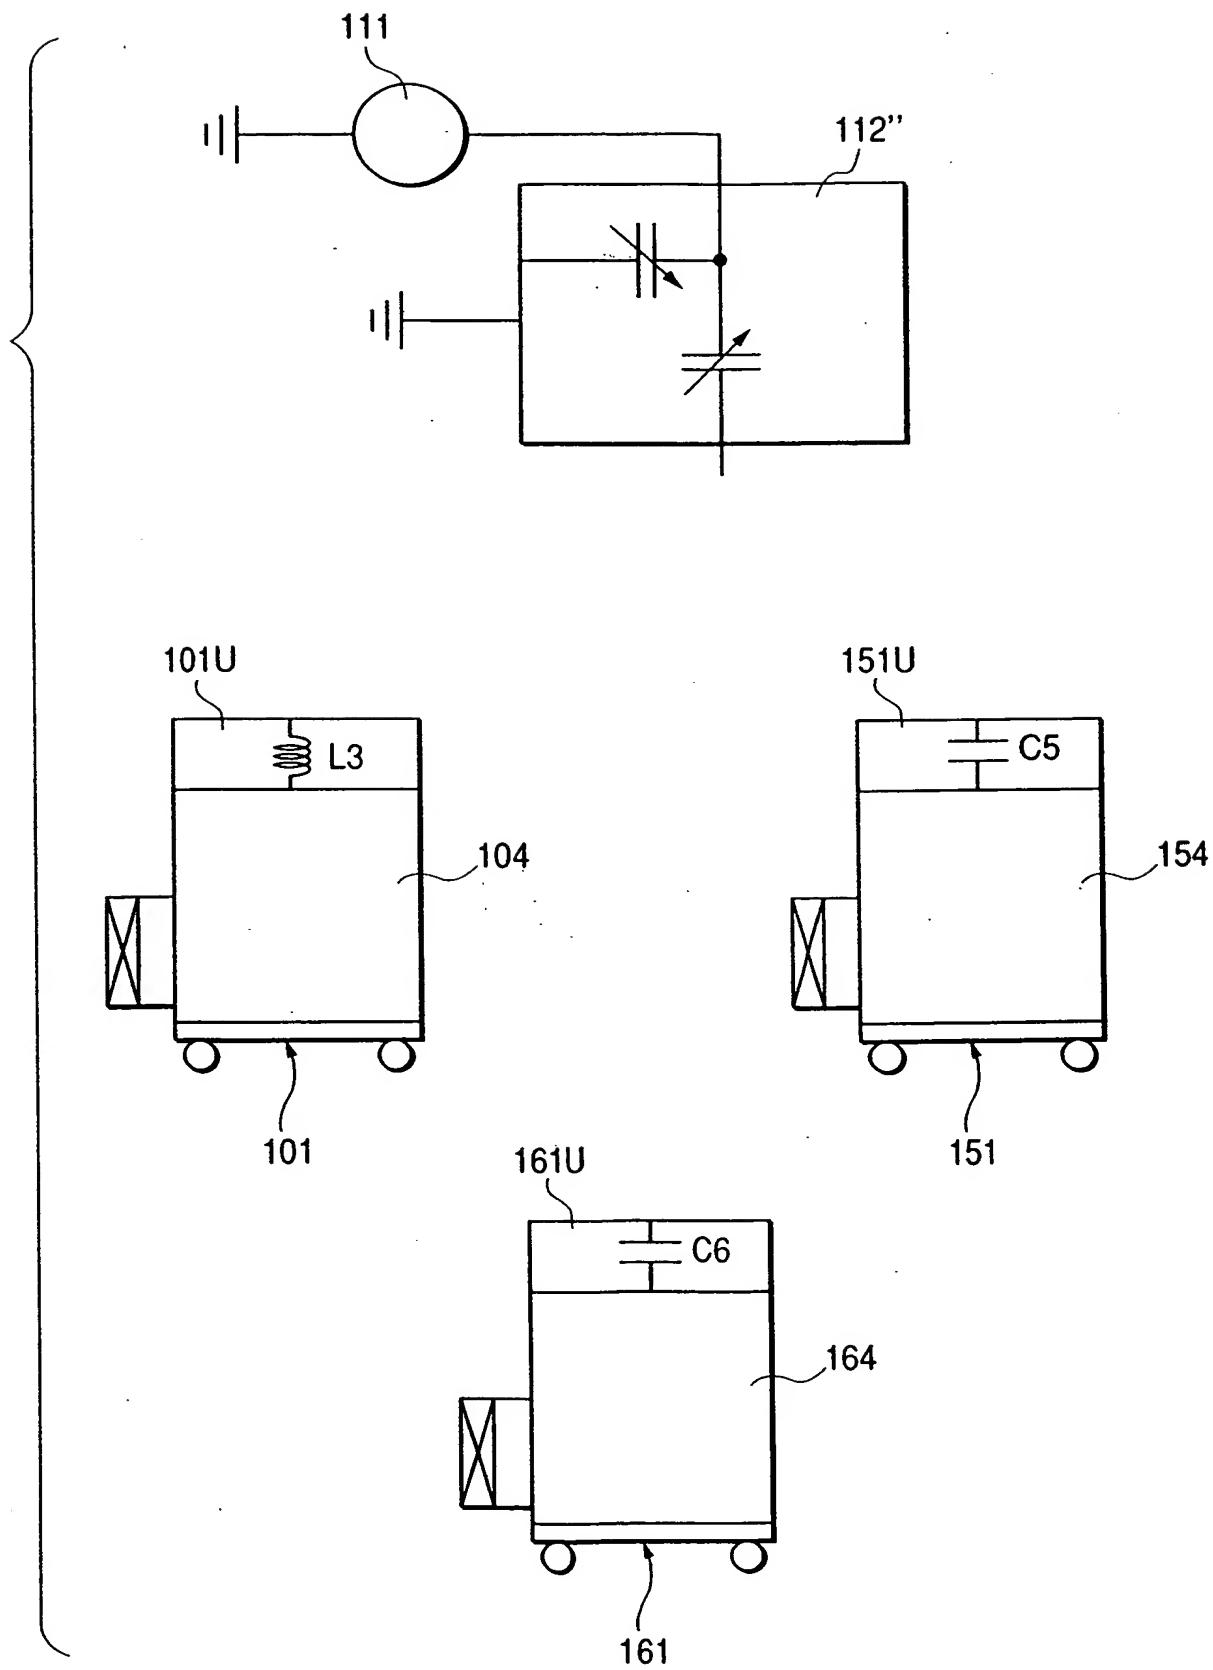


FIG. 6A

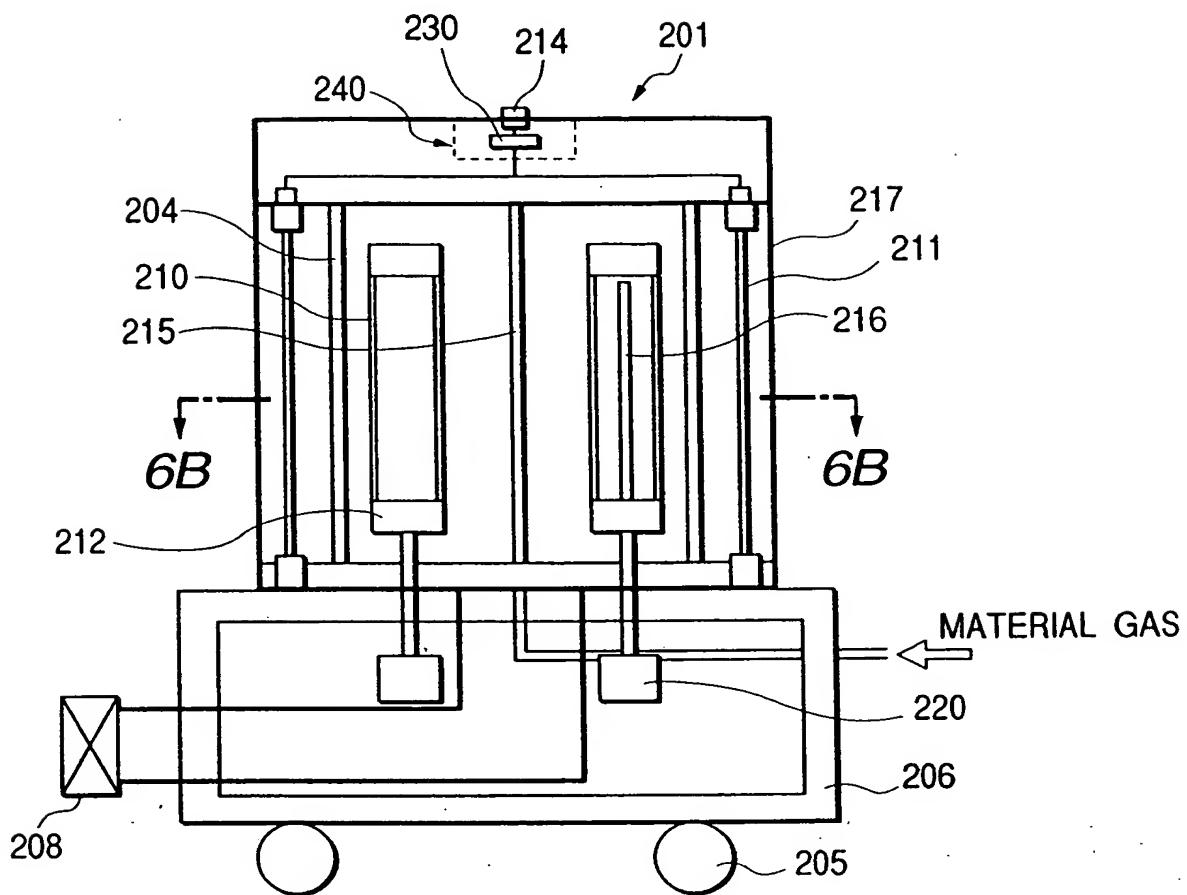


FIG. 6B

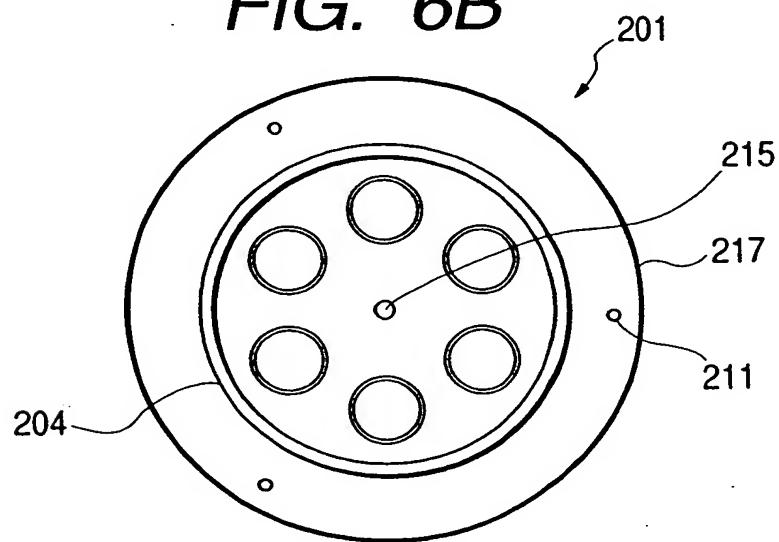


FIG. 7A

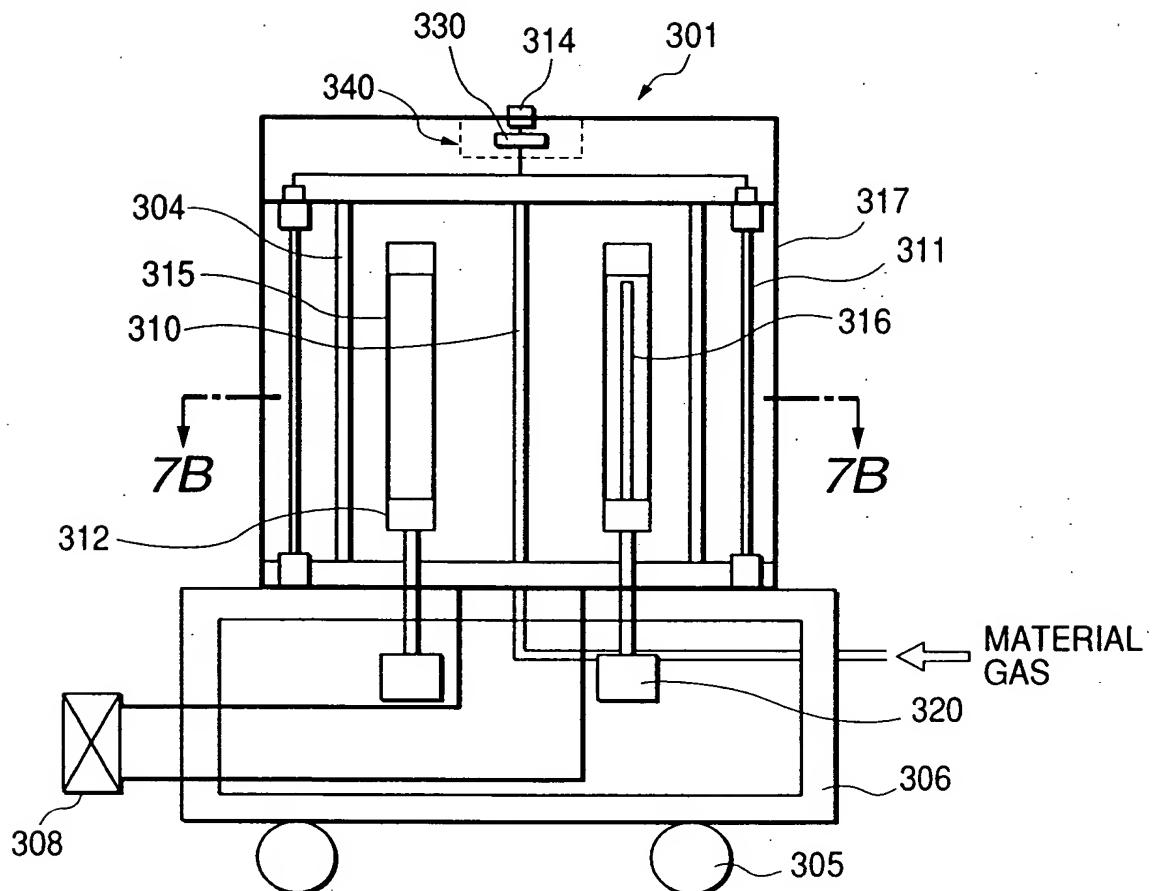


FIG. 7B

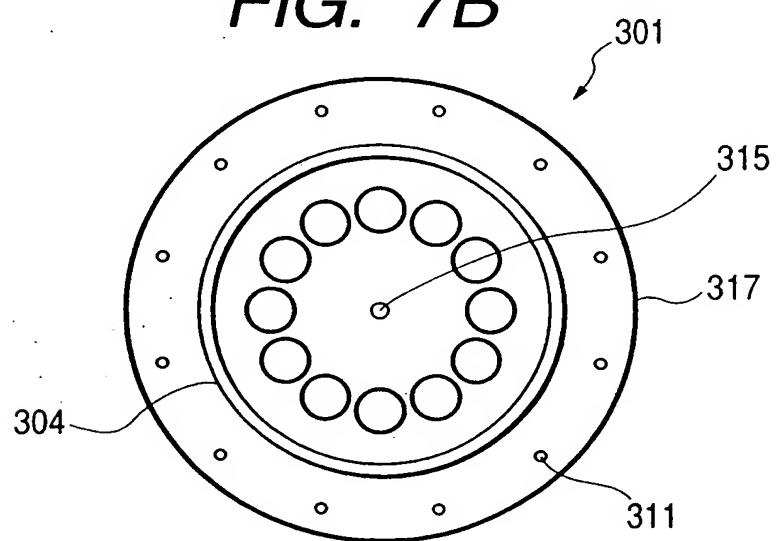


FIG. 8

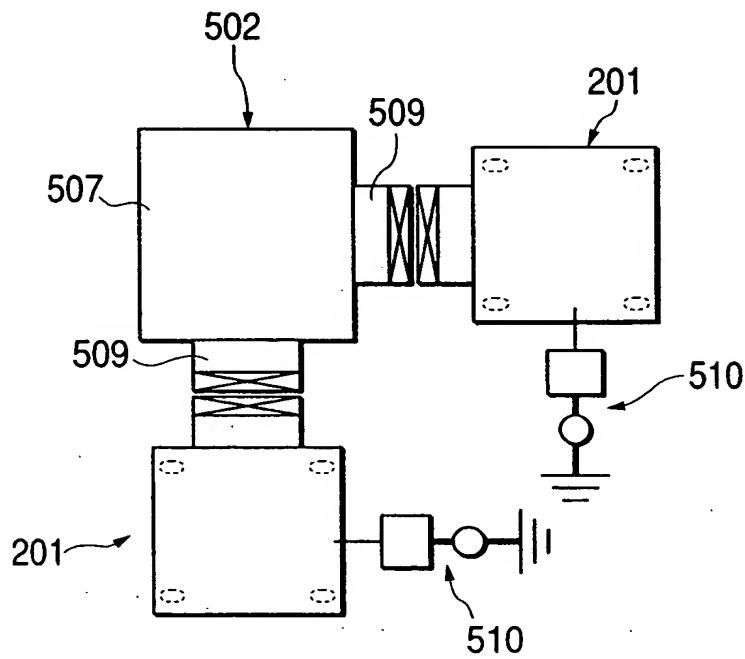
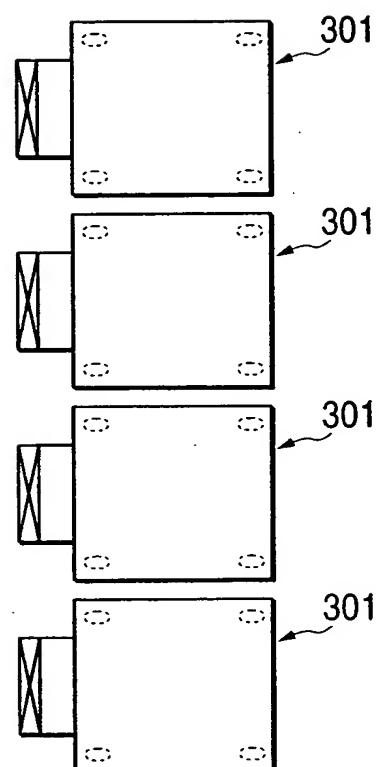
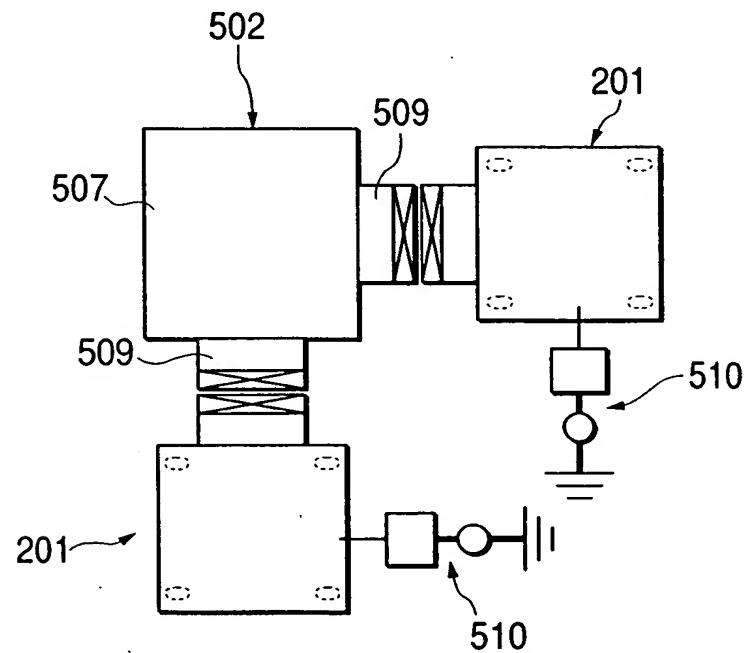
PLASMA TREATMENT AREAPLASMA TREATMENT AREA

FIG. 9

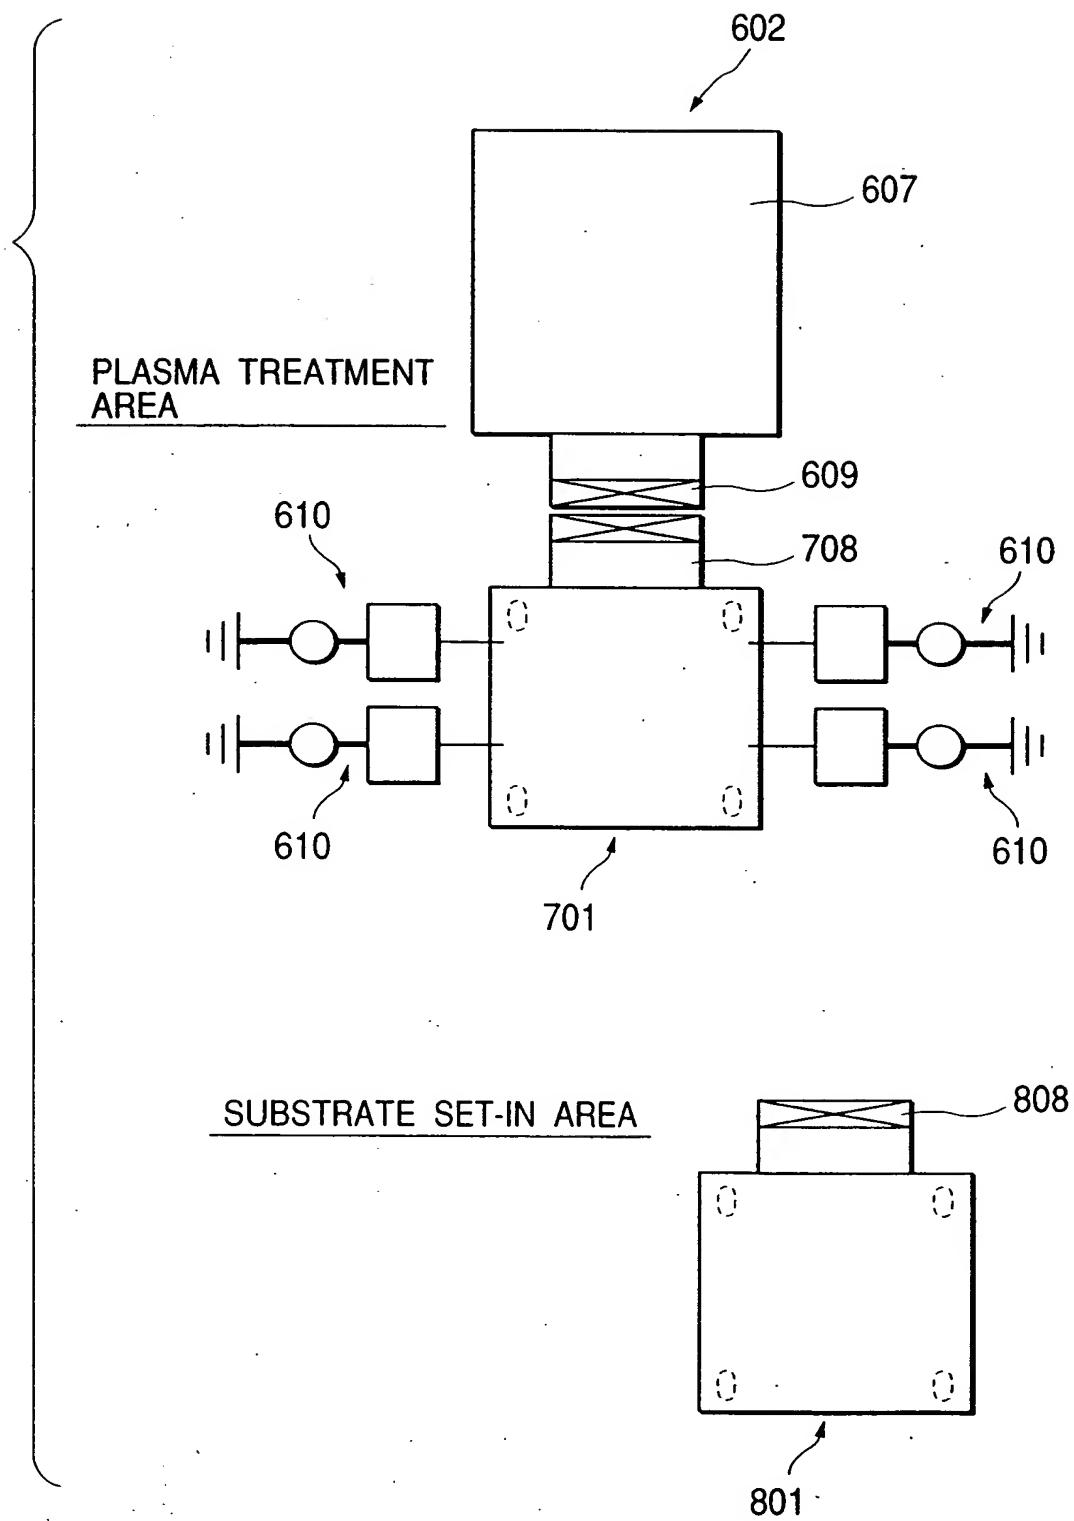


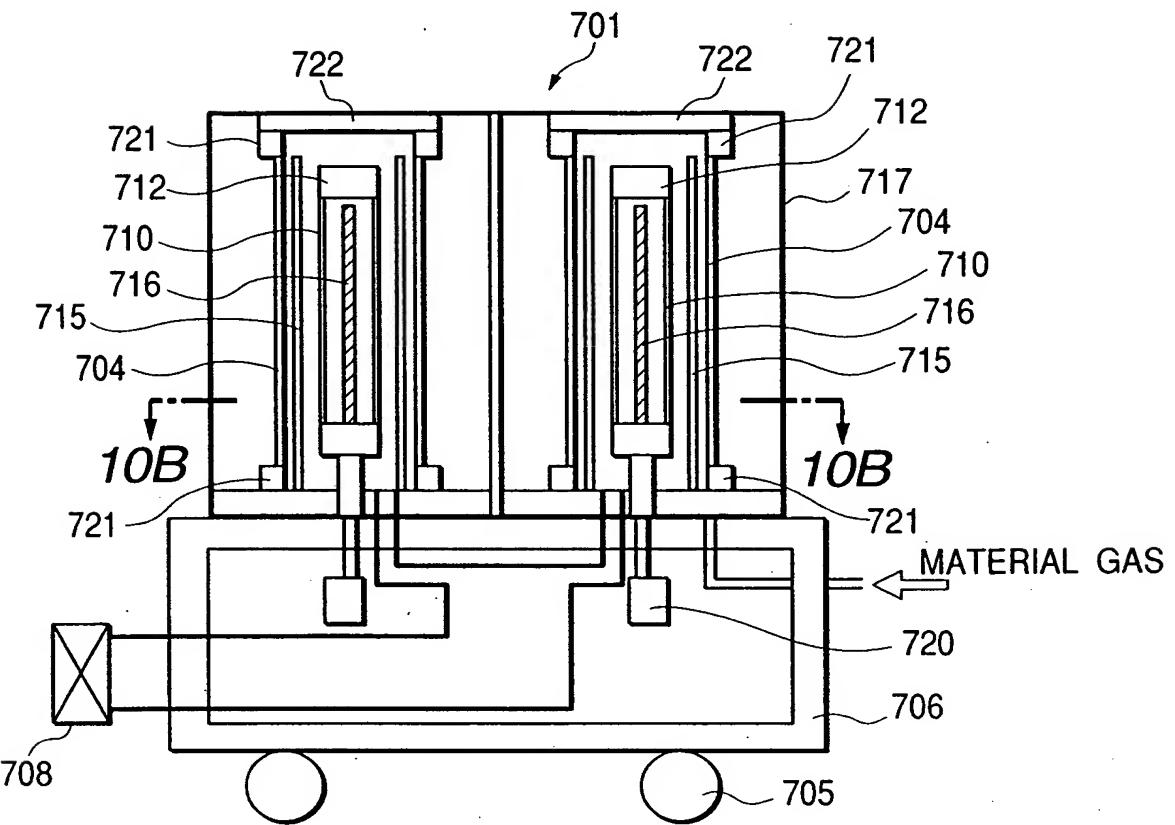
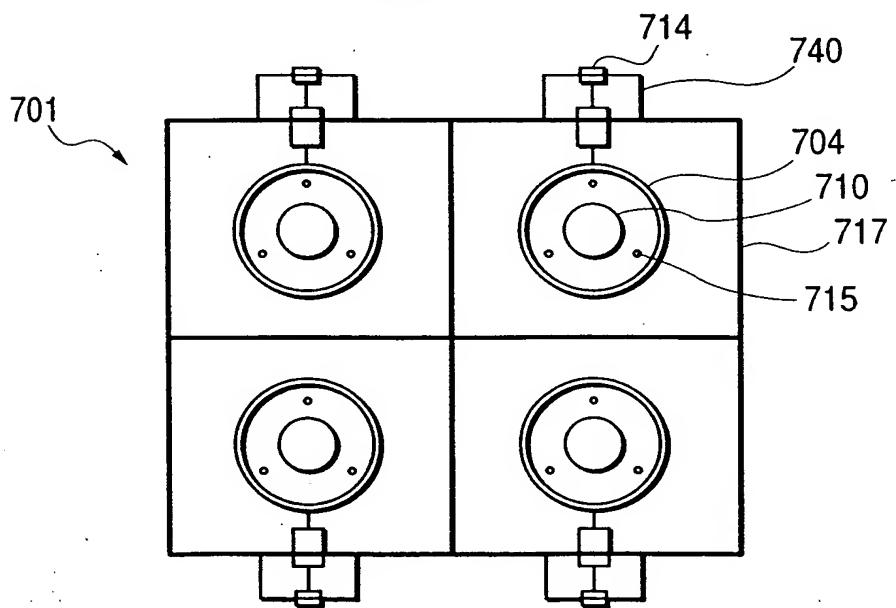
FIG. 10A**FIG. 10B**

FIG. 11A

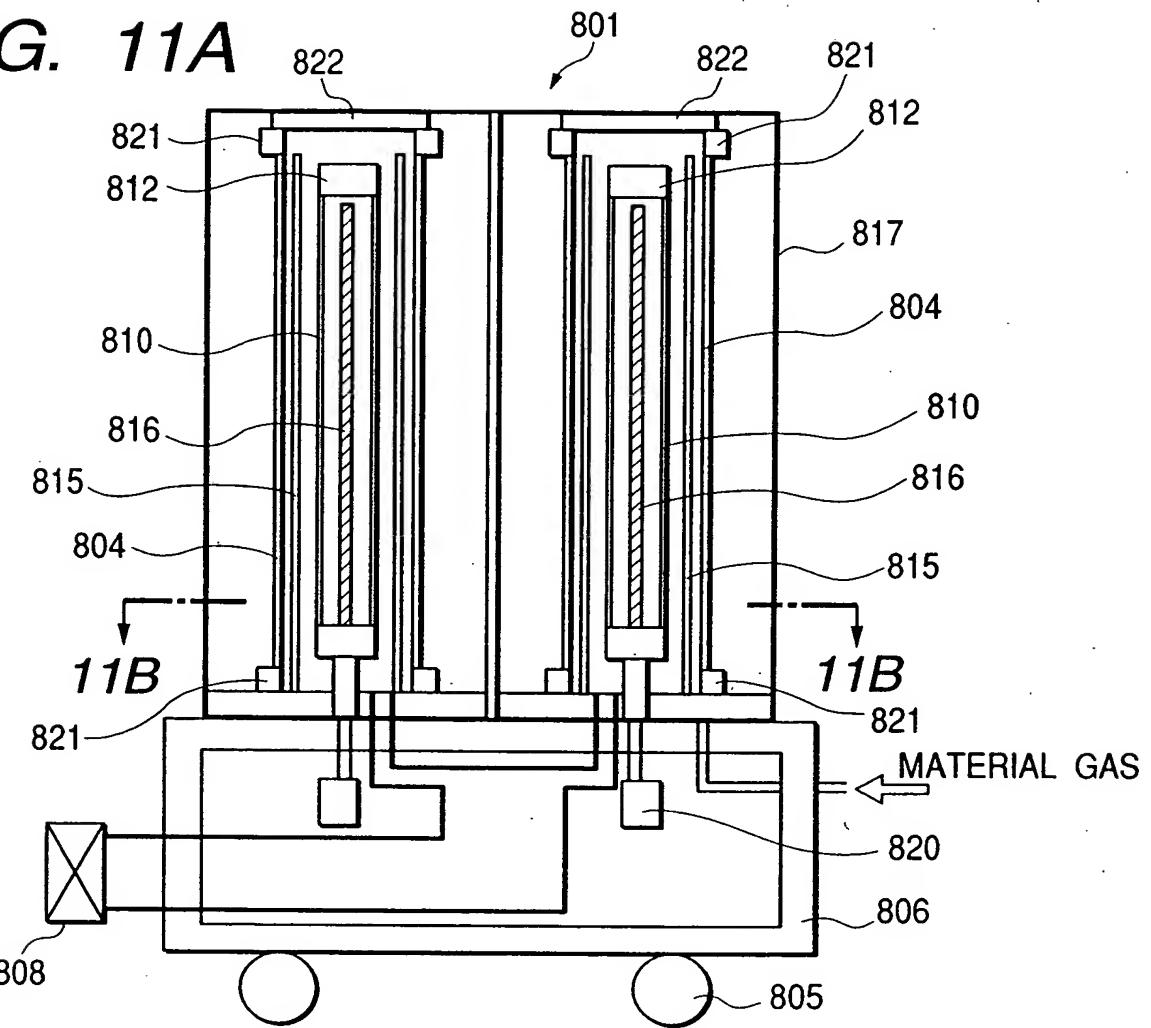


FIG. 11B

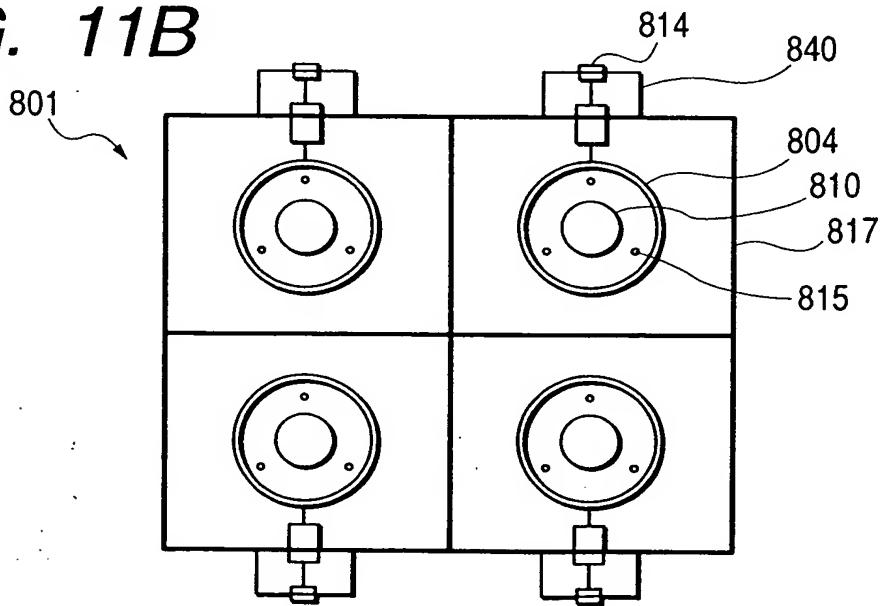


FIG. 12A

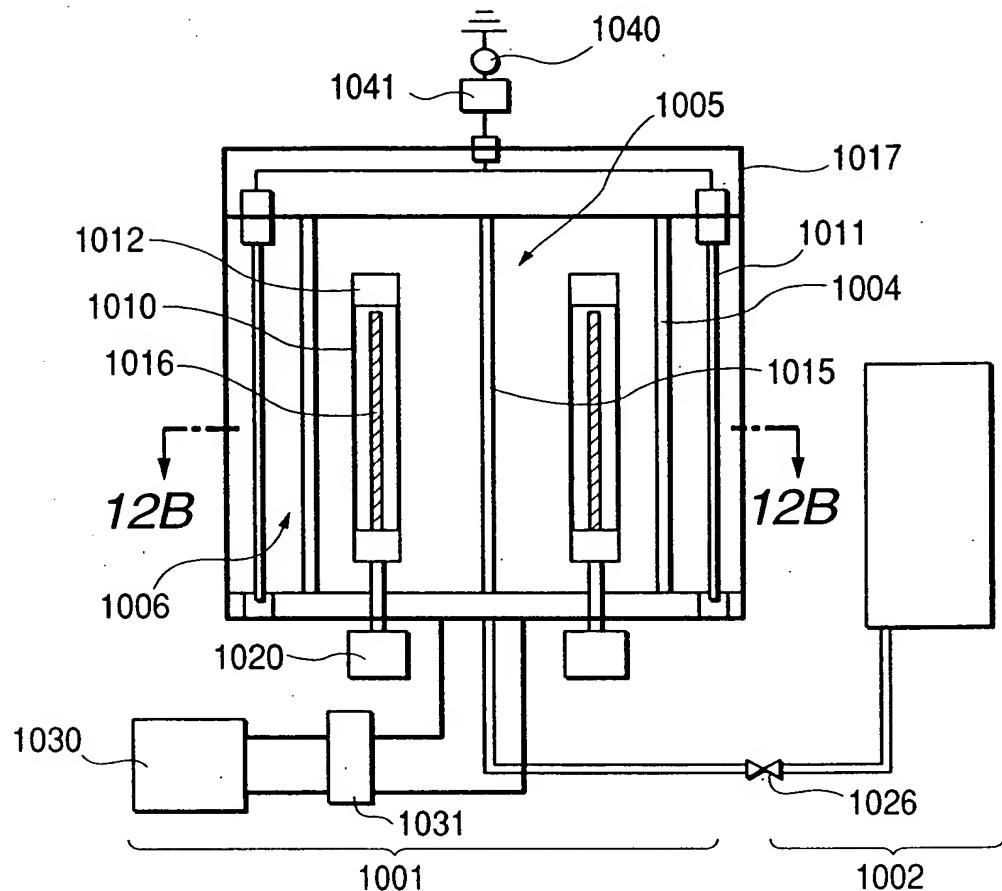


FIG. 12B

